


Listing of Equivalent Items available from **CHOICE ANALYTICAL** for use on AGILENT Models of ICP instrumentation

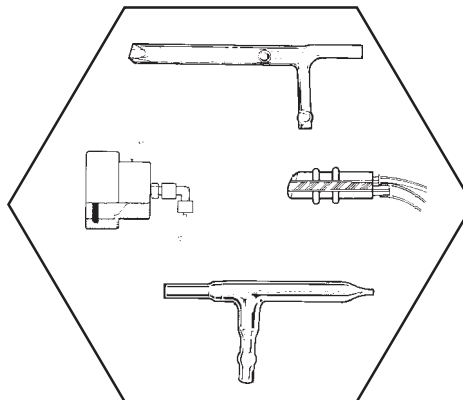

Nebulizer Listing for AGILENT Models ICP

Choice Analytical can supply both Genuine J.E. MEINHARD Nebulizers as well as a "Clone" type and SPECIAL TYPES for use on **AGILENT** models of instruments.

AGILENT Part No.	Part No. CHOICE	Description
------------------	-----------------	-------------

See attached pages for explanation of Descriptions and Types.

GENUINE J.E. MEINHARD ORIGINALS

TR-30-A0.5	"A" Type 0.5mlpm
TQ-30-A0.5	"A" Type 0.5mlpm, Quartz
TR-30-A3	"A" Type General Purpose
TR-30-C1	"C" Type
TR-30-C2	"C" Type
TR-30-C3	"C" Type for ICP-MS
TR-30-C0.5	"C" Type 0. mlpm
TR-50-C1	"C" Type for Hi Solid/Soln
TR-30-K2	"K" Type
TR-30-K3	"K" Type for Wear Metals

For other specifications and Special Application Types e.g. Small Bore, HEN (Hi-Efficiency), HPLC-MS etc. see attached sheets.

"CLONE TYPE"

	TR30-A0.5	Concentric Nebulizer A Type 0.5mlpm
	TR30-C0.5	Concentric Nebulizer C Type 0.5mlpm
	TR30-A0.5Q	Concentric Nebulizer A Type 0.5mlpm Quartz
	TR30-C0.5Q	Concentric Nebulizer C Type 0.5mlpm Quartz
	500-75	"A" Type Flush Tip 30 Psi 1ml/min
	500-76	"A" Type Flush Tip 30 Psi 2ml/min
G1820-65030	500-77	"A" Type Flush Tip 30 Psi 3ml/min (General Purpose)
G1820-65138	500-77Q	"A" Type Flush Tip 30 Psi 3ml/min Quartz
	500-71	"C" Type Recessed Tip 30 Psi 2ml/min
	500-70	"C" Type Recessed Tip 30 Psi 1ml/min (ICP-MS)
	500-72	"C" Type Recessed Tip 30 Psi 3ml/min (HiSolid)
	500-80	"K" Type (Wear Metals) 0.7 lpm Argon
	500-82	"K" Type, Trace
	500-90	"T" Type
G1820-65033	500-93	Nebuliser Crossflow
	4060-620	"C" Type Recessed Tip 42 Psi 2ml/min (0.4 L Ar/min)
	4060-610	"C" Type Recessed Tip 35 Psi 2ml/min (1.0 L Ar/min)



ctd. page 2

Nebulizer Listing for AGILENT Models ICP (ctd.)

Part No. AGLIENT	Part No. Choice	Description
<u>(MDSN) Hi-Solids — SPECIAL TYPES</u>		
G1820-65121	500-92	Nebulizer, Fixed Cross Flow
	500-93	Nebulizer, Fixed Cross Flow Hi-Solids
	510-10	Nebulizer, Noordermeer, V-Groove, MDSN
	510-50	Babbington V-Groove, MDSN (PEEK)
	520-30	Teflon End Cap for Spray Chambers
	520-40	Teflon End Cap for Babbington Nebulizer (510-50)
G1833-65475	520-42	End Cap Quartz
	520-424	End Cap Quartz
	4060-69	Teflon Parallel Path Nebulizer (Burgener)
<u>PFATYPE</u>		
G3139-8001	4060-010192	PFA Micro-flow Nebulizer 100ul/min
	4060-010600	PFA End Cap (No O-ring required)


Additional Items

520-35	Swagelok Fitting for Nebulizer Sample Inlet
520-36	Cross-Flow Nebulizer O-Ring for 500-92 & 500-93
520-37	Cross-Flow Nebulizer Teflon Sample Tube (2 foot = 61 cm)
520-38	Cross-Flow Nebulizer Argon Fittings for 500-92 & 500-93

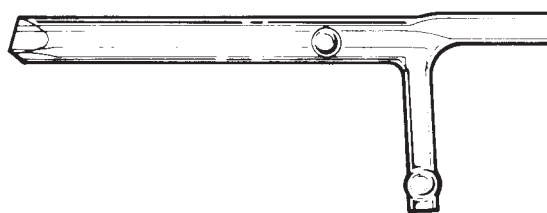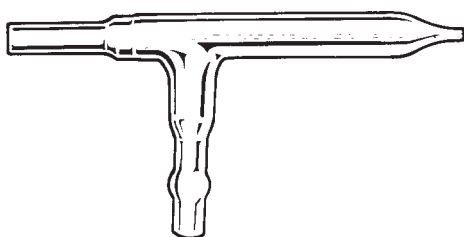


510-10 Nebulizer, Noordermeer, V-MDSN


- “CLONE TYPE”
 Concentric Nebulizers
 500-70 C-Type, Recessed Tip, 1mlpm
 500-71 C-Type, Recessed Tip, 2mlpm
 500-72 C-Type, Recessed Tip, 3mlpm
 500-75 A-Type, Flush Tip, 1mlpm
 500-76 A-Type, Flush Tip, 2mlpm
 500-77 A-Type, Flush Tip, 3mlpm
 500-80 K-Type, Nebulizer
 500-82 K-Type, Nebulizer, Trace

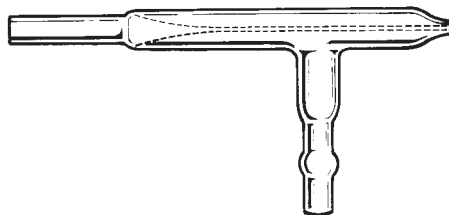


500-90 T-Type Nebulizer, Flush Tip



520-30 Teflon Endcap
for Spray Chambers



500-92 Fixed Cross-Flow
Nebulizer



510-50 Nebulizer,
Babbington V-Groove

AGILENT ICP Nebulizers [w] Page 2(2) 29/10/2007



CHOICE Analytical Pty Ltd

Supplies for Laboratory Instruments

Tel : + 61 2 9980 6240

Fax : + 61 2 9980 6344

ABN 66 052 203 719

E-mail : info@choiceanalytical.com.au

Web : www.choiceanalytical.com.au